

# SOIL MOISTURE METER

Model : DSMM500



Your purchase of this SOIL MOISTURE METER marks a step forward for you into the field of precision measurement. Although this METER is a complex and delicate instrument, its durable structure will allow many years of use if proper operating techniques are developed. Please read the following instructions carefully and always keep this manual within easy reach.

## OPERATION MANUAL

# TABLE OF CONTENTS

1. FEATURES.....	1
2. SPECIFICATIONS.....	1
3. FRONT PANEL DESCRIPTION.....	3
3-1 Soil moisture Probe.....	3
3-2 Moisture Sensing Head.....	3
3-3 Power Button.....	3
3-4 Hold Button.....	3
3-5 REC Button.....	3
3-6 LCD Display.....	3
3-7 Battery Compartment/Cover.....	3
4. MEASURING PROCEDURE.....	4
4-1 Measurement by selecting the different material.....	4
4-2 Data Hold.....	5
4-3 Data Record.....	5
5. BATTERY REPLACEMENT.....	6

## 1. FEATURES

- \* Designed to check the moisture level of soil or other similar material.
- \* Measurement range : 0 % to 50 % moisture content of soil sample with 0.1 % resolution.
- \* All in one digital soil meter, easy to make operation.
- \* Data hold function to freeze the desired value on display.
- \* Microprocessor circuit ensures high accuracy and provides special functions and features.
- \* Operates from DC 1.5V ( UM4/AAA ) x 4 PCs batteries.
- \* Built-in low battery indicator.
- \* Durable, long-lasting components, enclosed in strong, compact ABS-plastic housing.

## 2. SPECIFICATIONS

Applications	Designed to check the moisture level of soil or other similar material.
Measuring Principal	Used the 2 pins electrode to measure the conductive ability of the species, then converter to the reading of % " Moisture content " of soil sample.
Display	LCD size : 28 mm x 19 mm.

Measurement Range	0 % to 50 % moisture content on soil.
Resolution	0.1 %.
Accuracy	$\pm ( 5 \% + 5 d )$ F.S. <i>@ 23 °C <math>\pm</math> 5 °C, F.S. : full scale.</i>
Circuit	Custom one-chip of microprocessor LSI circuit.
Probe	2 pins moisture electrode.
Data Hold	Freeze the display reading.
Sampling Time	Approx. 0.8 second.
Operating Temperature	0 to 50 °C .
Operating Humidity	Less than 80% R.H.
Power Supply	DC 1.5 V battery ( UM4/AAA ) x 4 PCs,
Power Current	Approx. DC 5 mA
Weight	267 g/ 0.58 LB. <i>@ Battery is included.</i>
Dimension	<i>Meter body :</i>
	172 x 40 x 40 mm ( 6.8" x 1.6" x 1.6" ).
	<i>Probe body :</i>
	202 mm x Dia. 10 mm 8" x Dia. 0.4" .
	<i>Total length ( meter + probe ) :</i>
	374 mm ( 14.7 " ).
Accessories Included	Instruction manual..... 1 PC.

### 3. FRONT PANEL DESCRIPTION

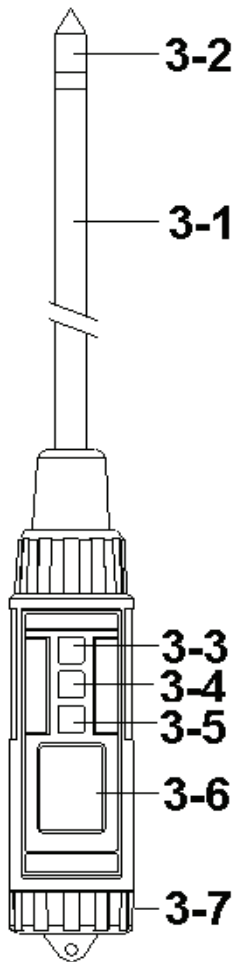


Fig. 1

- 3-1 Soil moisture Probe
- 3-2 Moisture Sensing Head
- 3-3 Power Button
- 3-4 Hold Button
- 3-5 REC Button
- 3-6 LCD Display
- 3-7 Battery Compartment/Cover

## 4. MEASURING PROCEDURE

### 4-1 Soil measurement

1) Turn on the meter by pressing the " Power Button "  
( 3-3, Fig. 1 ) momentarily.

*\* Press the " Power Button " ( 3-3, Fig. 1 )  
momentarily again will turn off the meter.*

2) Insert the " Moisture sensing head " ( 3-2, Fig. 1 ) into  
the measured soil.

**It is recommended that probe head should be  
inserted into the soil at least 10 cm when make  
the measurement..**

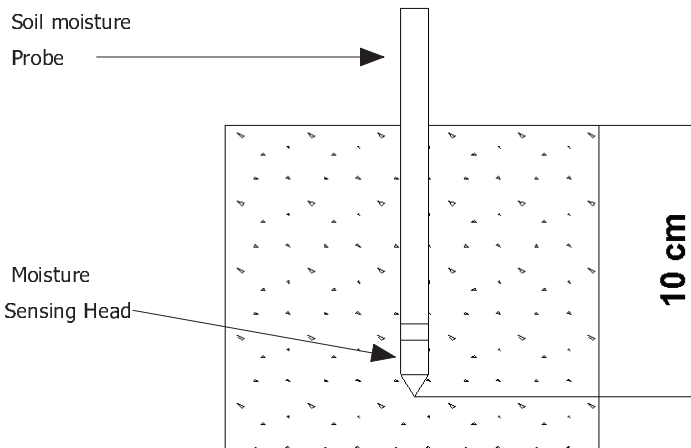


Fig. 2

### ***Consideration :***

***If the sample soil under testing has a high  
moisture content it may take a few minutes to  
obtain a stable reading.***


#### **4-2 Data Hold**

- \* During the measurement, press the " Hold Button " ( 3-4, Fig. 1 ) momentarily to hold the measured value. The LCD will show a " HOLD " symbol.
- \* Press the " Hold Button " once again to release the data hold function.

#### **4-3 Data Record ( Max., Min. reading )**

- 1) The data record function records the maximum and minimum readings. Press the " REC Button " ( 3-5, Fig. 1 ) momentarily to start the Data Record function, shows " REC " on the display.
- 2) With the " REC " symbol on the display.
  - a) Press the " REC Button " ( 3-5, Fig. 1 ) momentarily, the " REC MAX " symbol along with the maximum value will appear on the display.
  - b) Press the " REC Button " ( 3-5, Fig. 1 ) momentarily again, the " REC MIN " symbol along with the minimum value will appear on the display.
    - \* When display shows " REC MAX " or " REC MIN ", press the " Hold Button " ( 3-4, Fig. 1 ) momentarily will delete the max. ( min. ) value, the display will show the " REC. " only and execute the memory function continuously.*
- c) To exit the memory record function, press the " REC " button for 2 seconds at least. The display will revert to the current reading, not show " REC "

## 5. BATTERY REPLACEMENT

- \* Replace the batteries when the left corner of the LCD displays the low battery icon " , using 4 fresh 1.5 V ( UM4, AAA ) batteries.
- \* To change the batteries, open ( rotate clockwise direction ) the " Battery Cover " ( 3-7, Fig. 1 ).
- \* Make sure the " Battery cover " (3-7, Fig 1) is secured after changing the batteries.



**Specialty Tools & Instruments™**

---

**GENERAL TOOLS & INSTRUMENTS™**

80 White Street  
New York, NY 10013-3567  
PHONE (212) 431-6100  
FAX (212) 431-6499  
TOLL FREE (800) 697-8665

e-mail: [sales@generaltools.com](mailto:sales@generaltools.com)  
[www.generaltools.com](http://www.generaltools.com)

DSMM500 User's Manual

Specifications subject to change  
without notice

©2009 GENERAL TOOLS & INSTRUMENTS™

NOTICE - WE ARE NOT RESPONSIBLE FOR TYPOGRAPHICAL ERRORS.

MAN#DSMM500 04/09